

10074512.021102





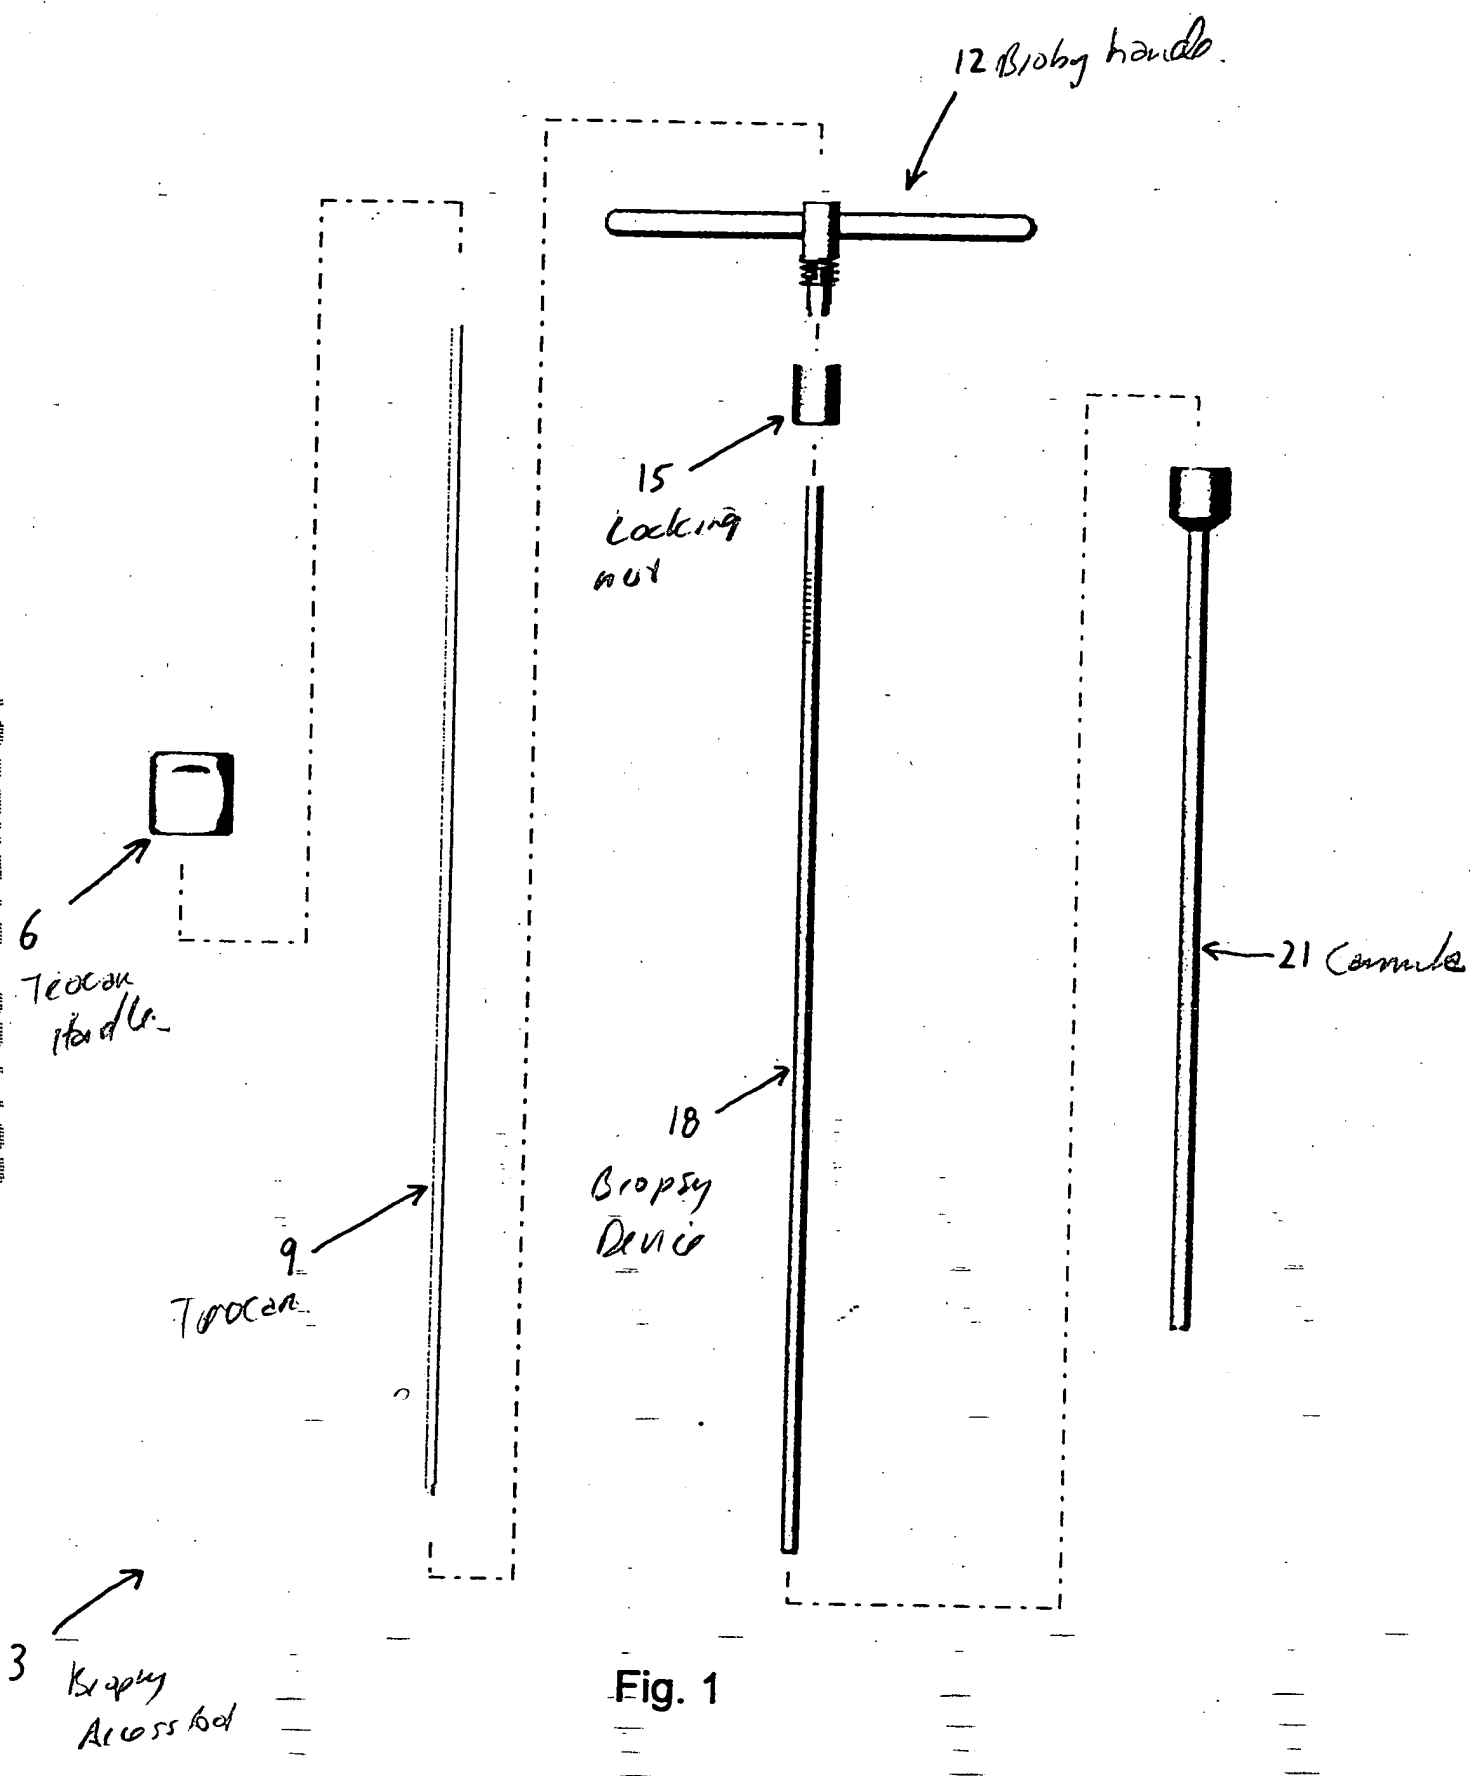


Fig. 1

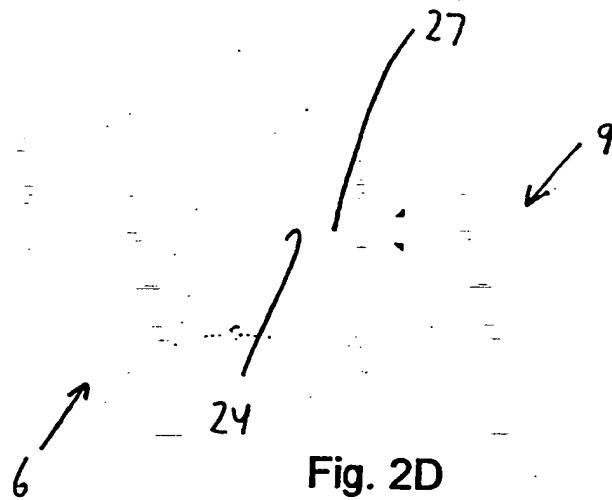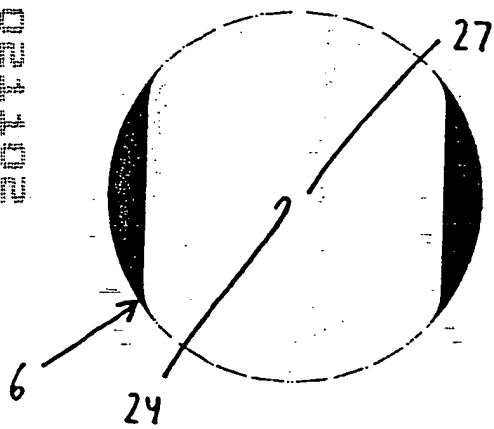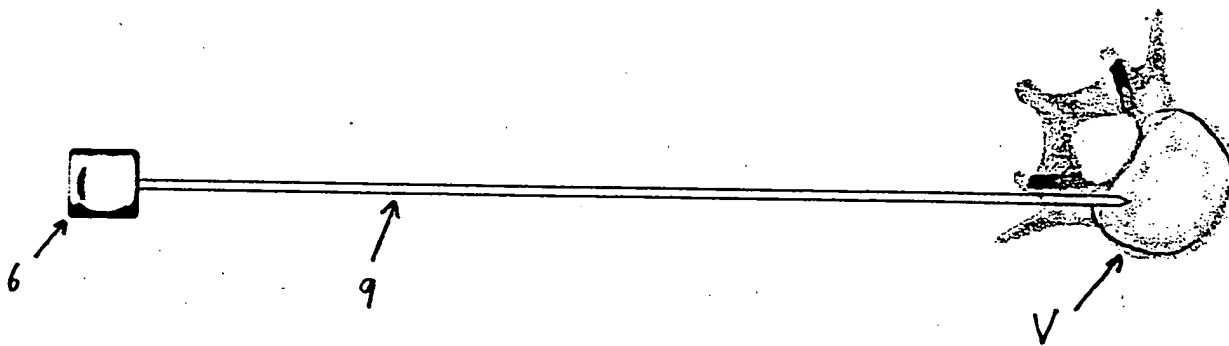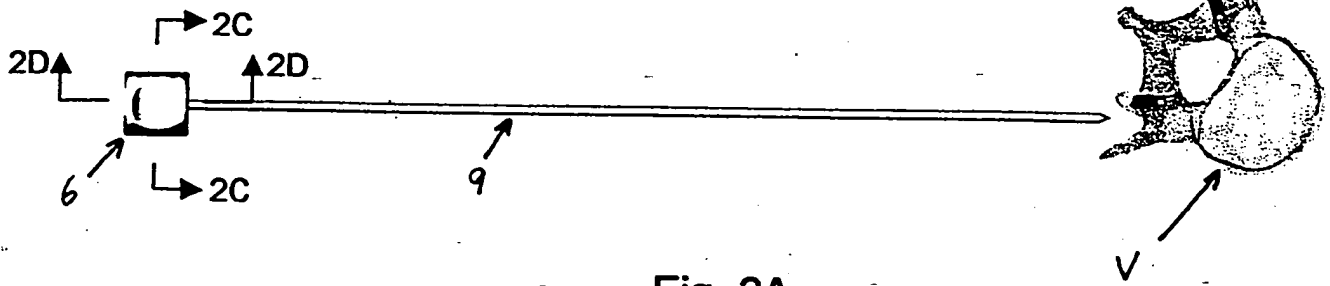

10074512.024102

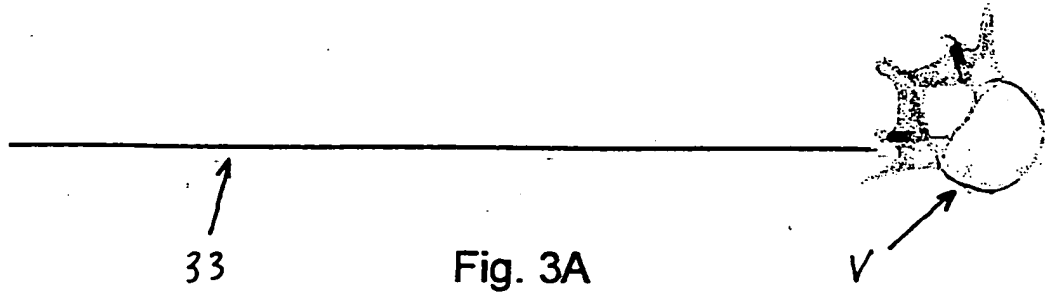


Fig. 3A

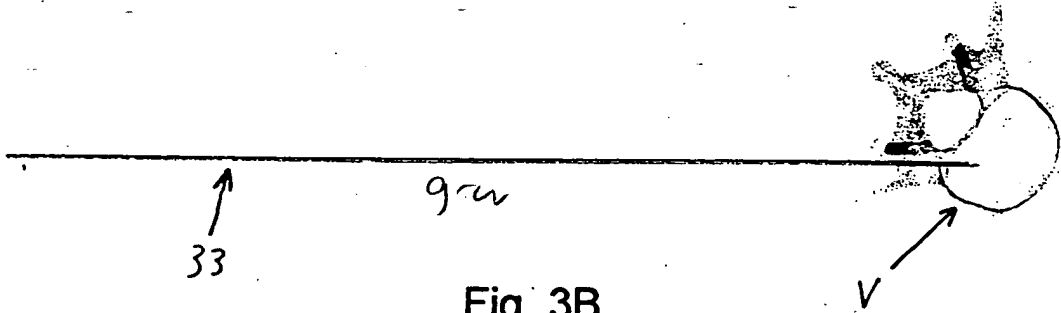


Fig. 3B

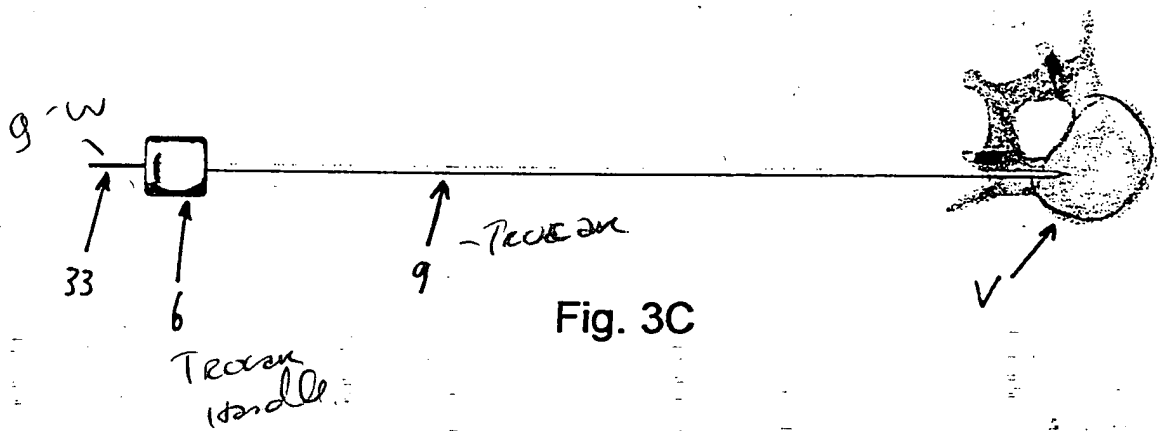


Fig. 3C




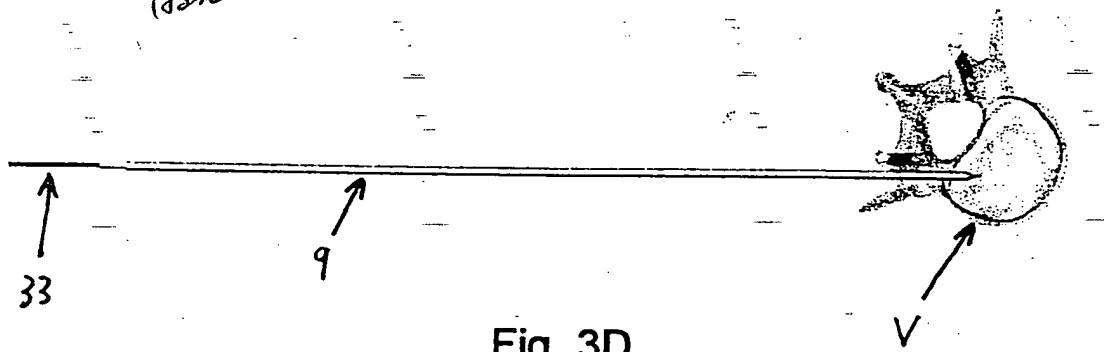


Fig. 3D

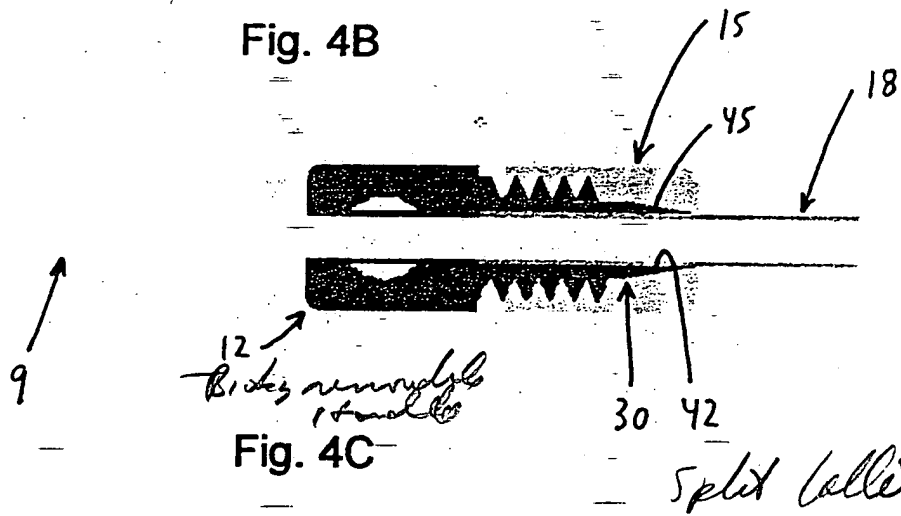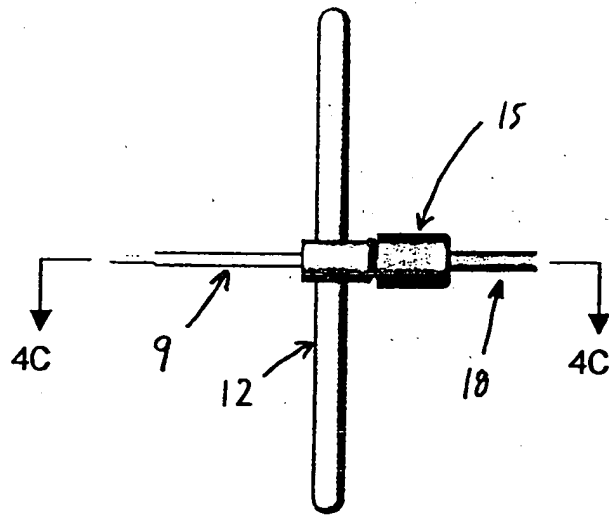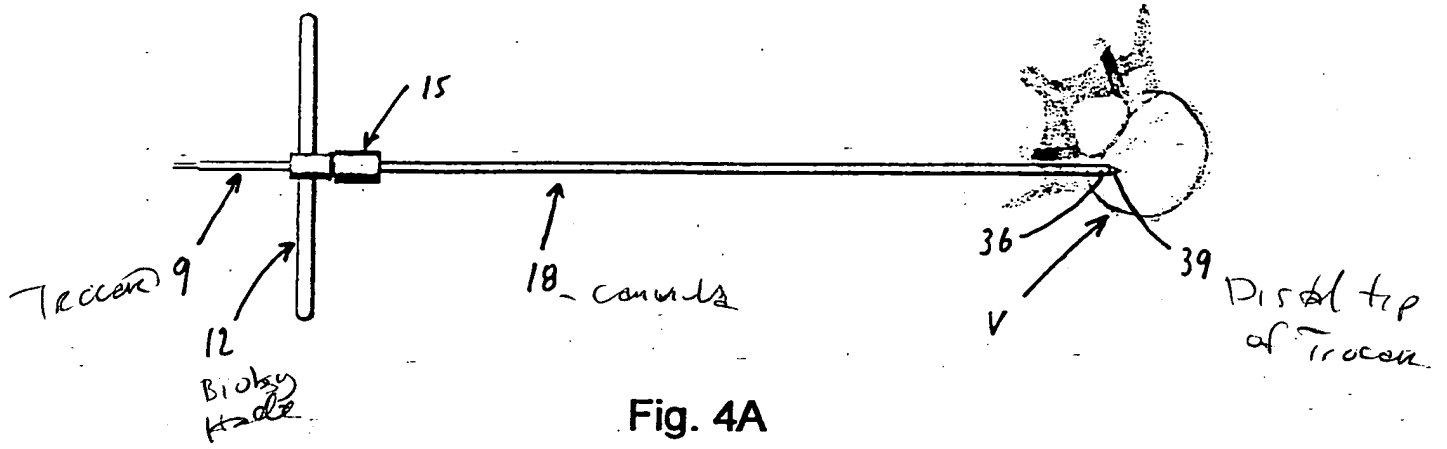

10074512-02102

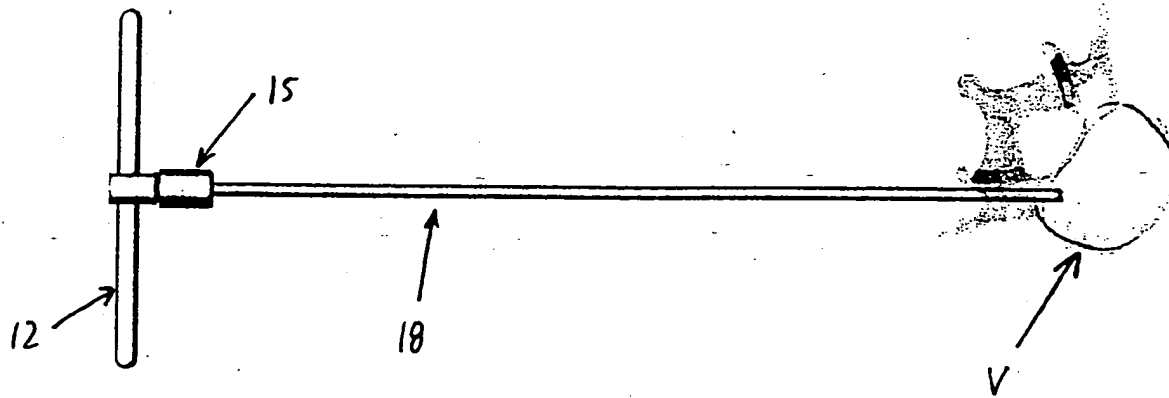


Fig. 5



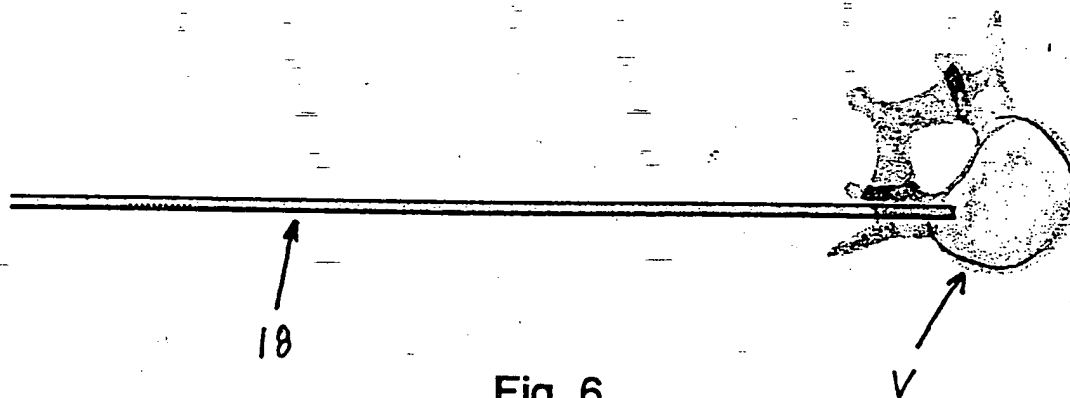


Fig. 6

2017-02-20 15:42:00

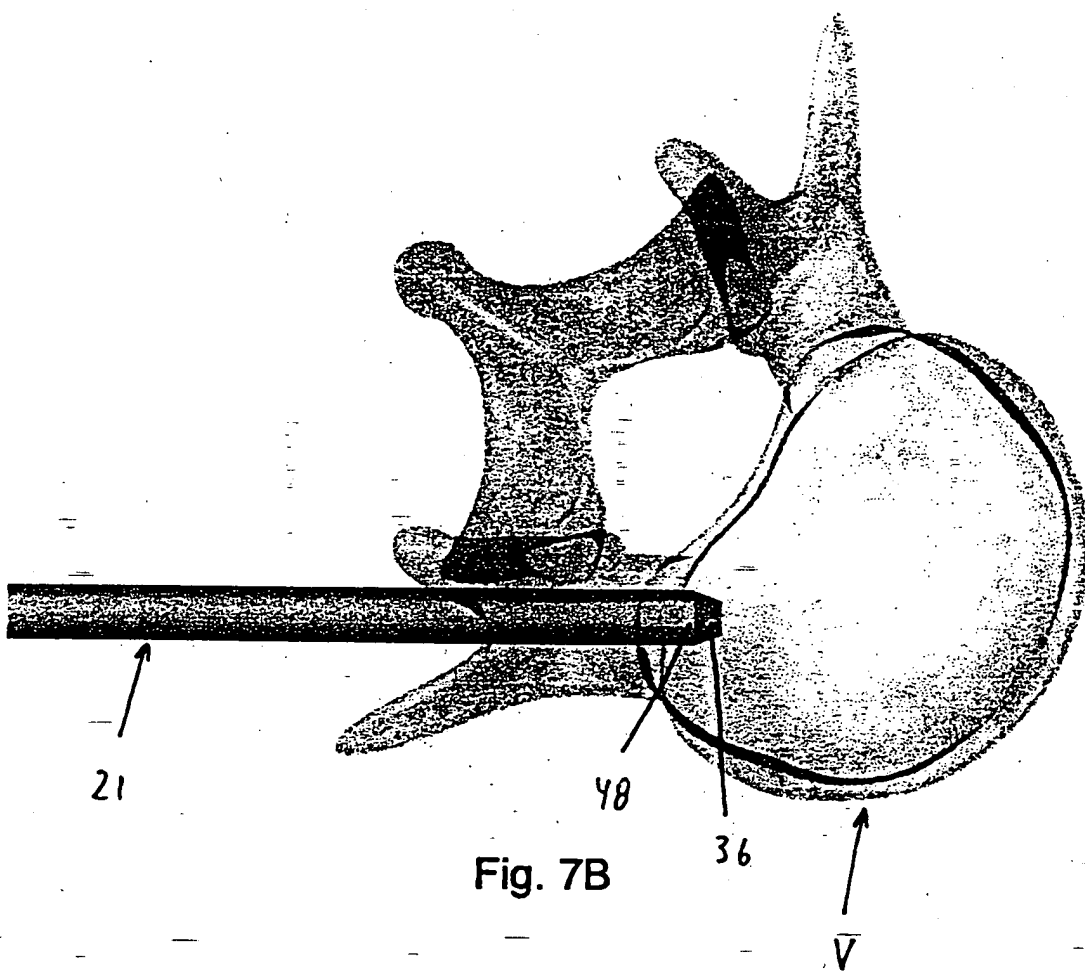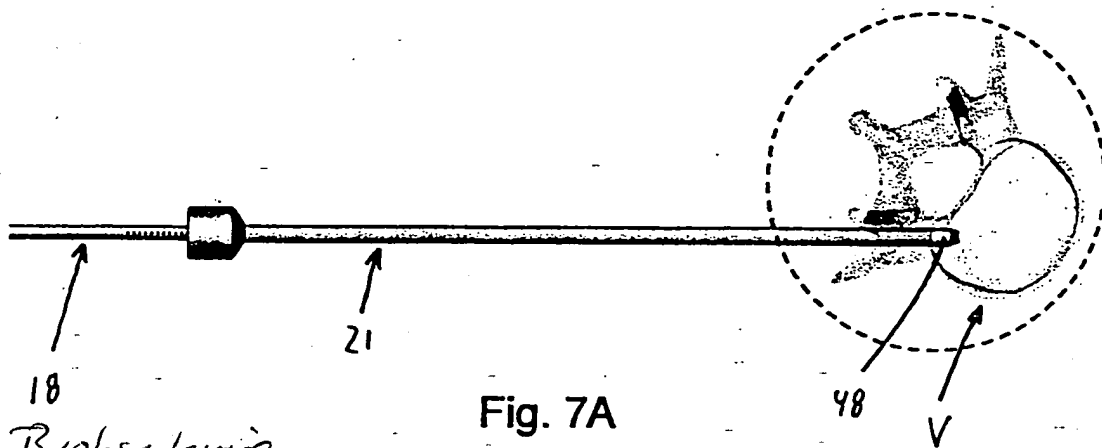

Biopsy device

2014512-021100

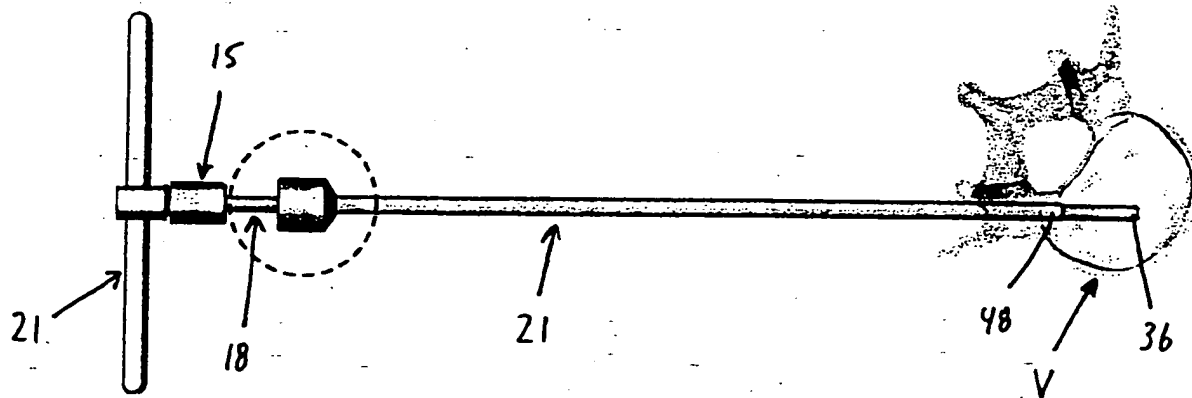


Fig. 8A

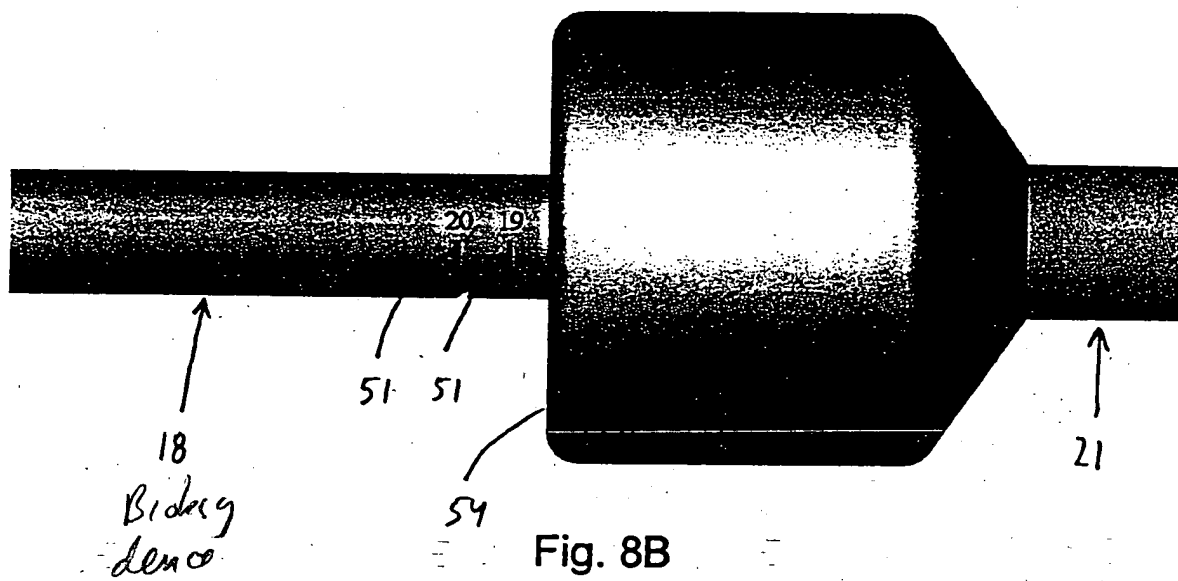


Fig. 8B


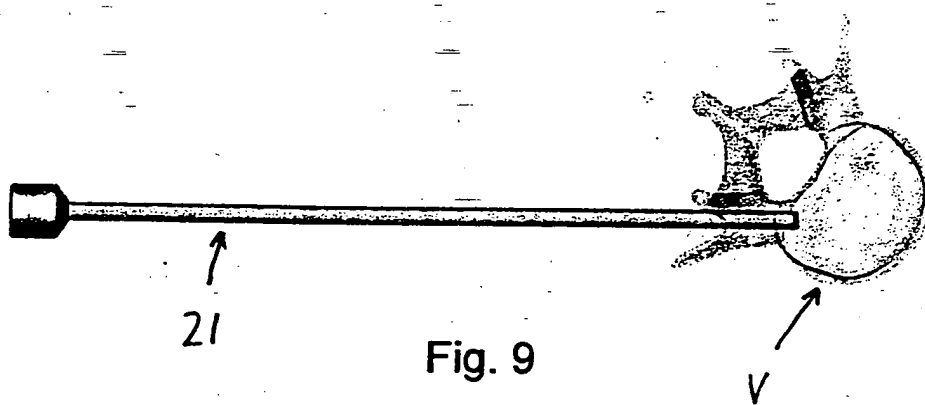


Fig. 9

10074512-024102

20172012154200T

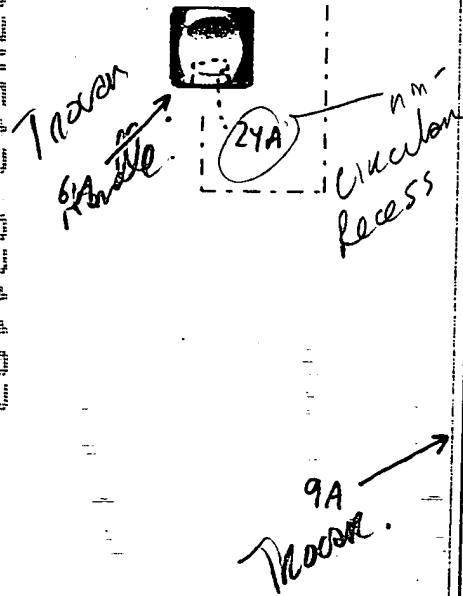

3A

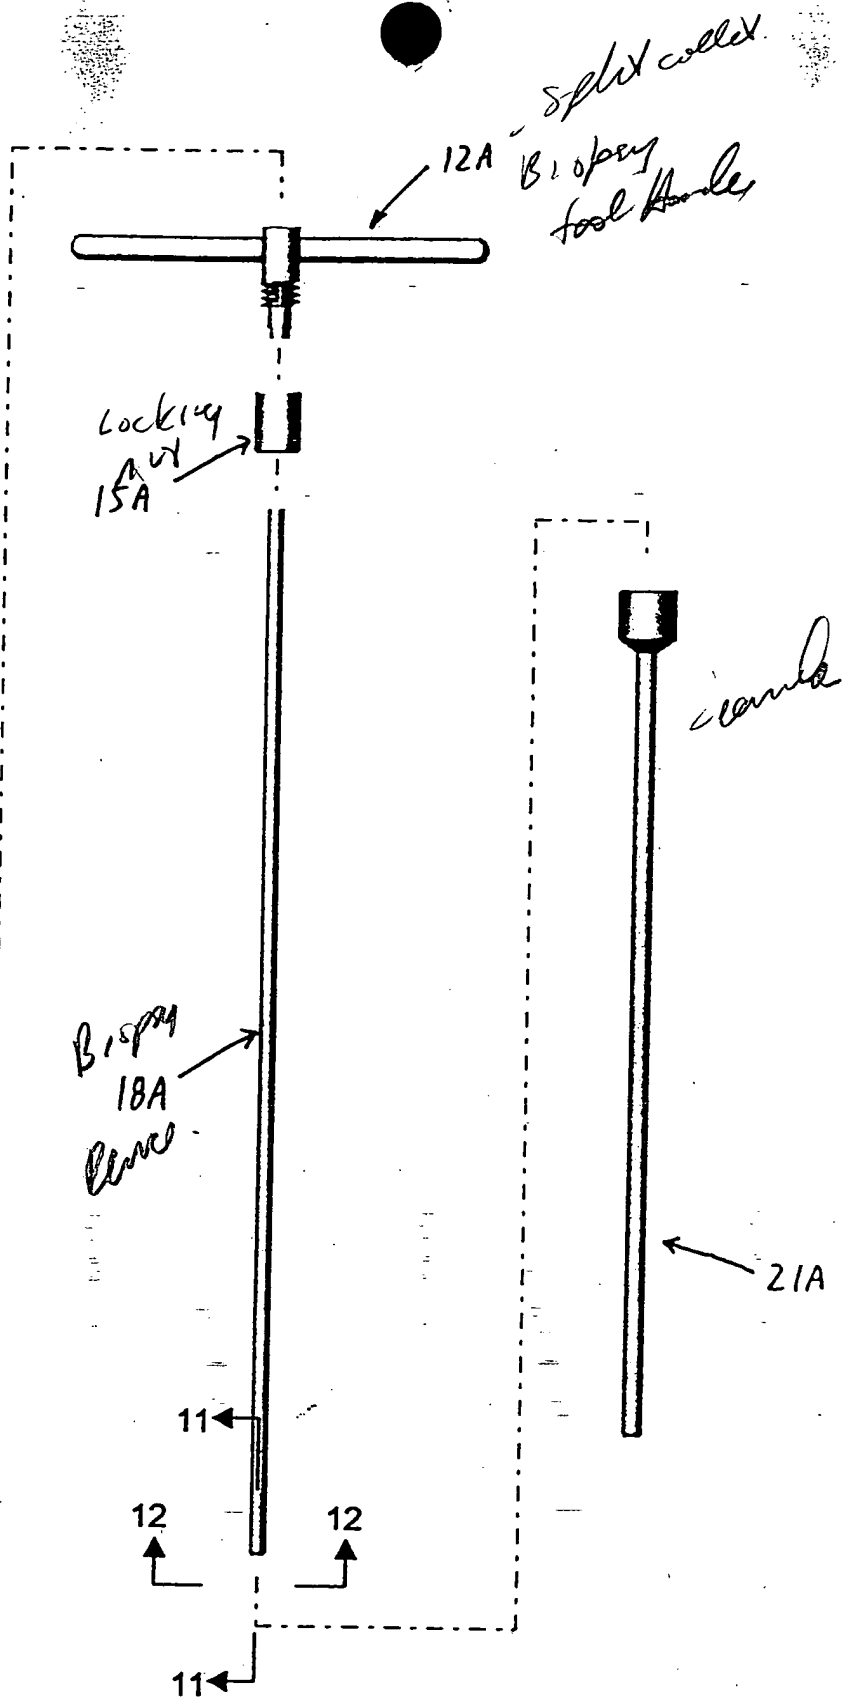


Fig. 10



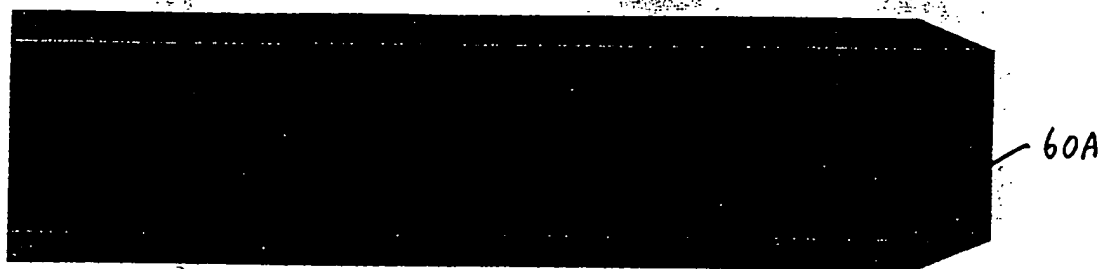


Fig. 11

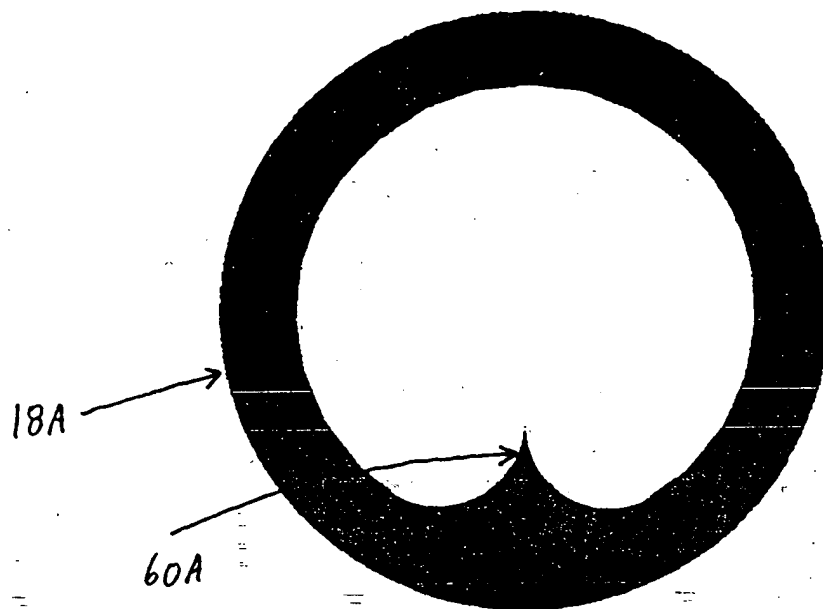


Fig. 12

10074512-024102

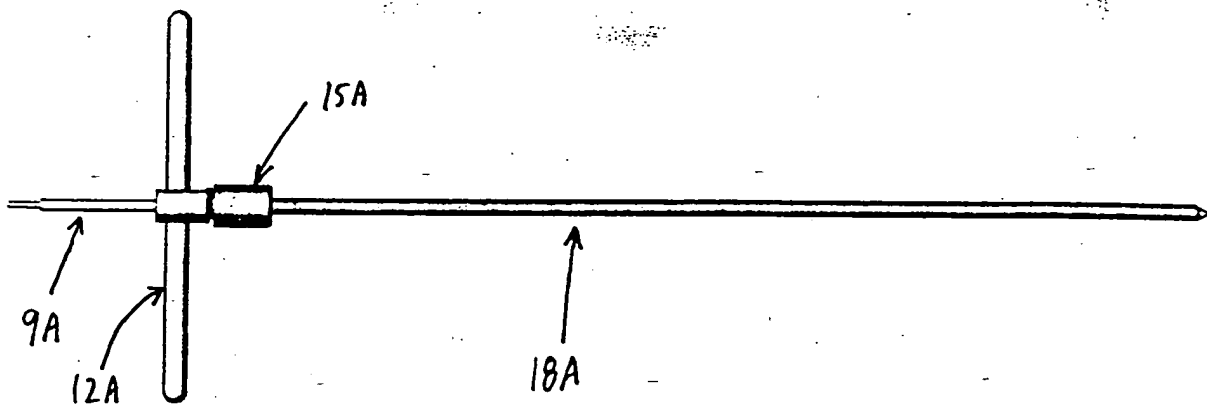


Fig. 13A

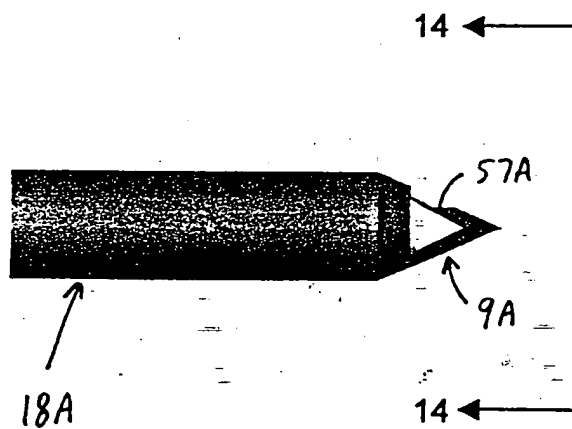


Fig. 13B

201720-2154200T

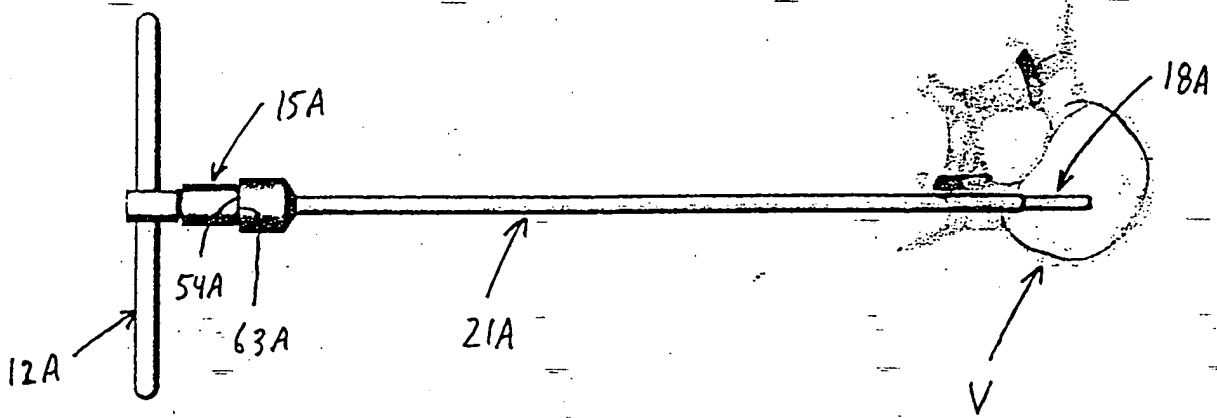


Fig. 14

10074512.021102